

PRO SERIES

EXTERNAL DUAL DEEP LOW TEMPERATURE RECORDER

WS-T21SLPRO

Product Overview:

Wason PRO series temperature and humidity recorder is a single model of precision instrument for automatic data storage. The instrument adopts low power consumption design, long standby time; Double cavity structure, high waterproof grade; adaptable to different sensors, wide detection range. C-mi software can be used to achieve parameter setting, data download, data analysis, data export and other functions, and can directly copy data in CSV format from the logger without using C-mi software. Widely used in food and medicine, cold chain logistics, chemicals, electronics, archives, agricultural research and other fields.

Product Characteristics:

- 1) No special software is required to download data;
- 2) Different probe applicable;
- 3) Multi-process mode;
- 4) °C/°F switch able;
- 5) Host with IP65 waterproof grade, suitable for harsh environment;
- 6) Low power design, battery life: 1 ~ 2 years;
- 7) ABS engineering plastic shell, with double chamber;
- 8) LCD display: temperature, time, battery capacity, alarm, etc.



Product Parameter:

Sensor type	Deep low temperature (external)
Number of sensors	Dual channel
Sensor length	1.5m
Temperature range	-200°C~0°C
Temperature accuracy	(-20~70) °C: ± (0.3~0.5) °C; Other: ±1°C
Display resolution	(-99.9~0) °C: 0.1°C/0.1°F; Other: 1°C /1°F
Memory resolution	(-99.9~0) °C: 0.1°C/0.1°F; Other: 1°C /1°F
Recording capacity	64800 groups
Record interval	1min~60min
Parameter configuration	Special software configuration, manual key configuration

Out-of-limit alarm	LCD prompt, buzzer alarm
Clock	Real-time clock display
Starting mode	Manual start, the software starts periodically
Stop mode	Manual stop, full stop
Communication interface	Mini USB
Power supply	High energy lithium battery
Battery life	1~2 years (depending on frequency of use)
Host operating environment	-20℃~70℃
Overall dimension	93mm×62mm×22mm
Weight	108g
Calibrate	Standard product with factory calibration certificate, optional accessory with CNAS calibration certificate
Shell material	ABS(shock-resistant)
Keep under warranty	12 months
Class of protection	IP65
Product certification	CE certification

Product Accessories:

Accessories			
Name	External deep low temperature temperature sensor	USB Data cable	User manual
Type	P005	P108	/
Accessories			
Name	Calibration certificate	Software Get Business Card	Lithium battery
Type	/	/	P701


Accessories			
Name	CNAS Calibration Certificate		
Type	/		
Note information	Optional		

Usage Method:

Method 1:

None-driving usage (no special software required, more convenient to use, the third generation recorder unique use mode.)


- ①According to the instructions, parameters are set by four buttons on the recorder.
- ②After the setting is completed, place it in the environment to be detected, and open the record.
- ③Stop recording, connect it to the computer with a USB cable to download the data.
- ④Copy data files in CSV format directly from the recorder, which can be opened by text processing software such as EXCEL or TXT.

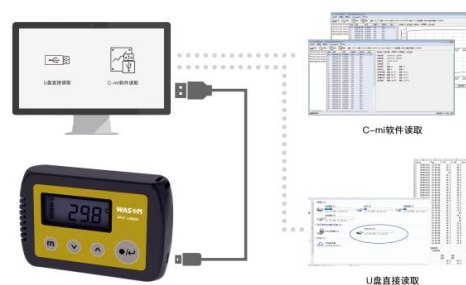

Method 2:

When you have more requirements for data analysis, please use the dedicated software to download the data, through the dedicated software you can view data reports, data curves, data statistics, record remarks and other information, but also output PDF data files.


- ①Copy the special software to your computer, green software, no need to install, open to use.
- ②Connect the recorder to the computer and set parameters when the recording is stopped.
- ③Remove the recorder from the computer, and place it in the environment that needs to be detected, and turn it on.
- ④Stop recording, connect the recorder to the computer, check historical data, historical curves, data statistics, etc., and print data, output PDF and other format files.

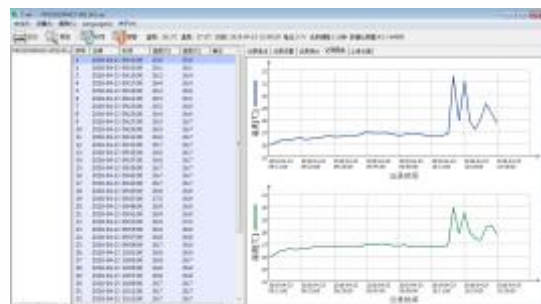

序号	日期	时间	温度T1	温度T2	湿度
1	2018-04-19	11:00:00	22.5	22.2	22.8
2	2018-04-19	11:14:00	22.7	22.7	22.7
3	2018-04-19	11:16:00	22.8	22.8	22.8
4	2018-04-19	11:18:00	22.8	22.8	22.8
5	2018-04-19	11:20:00	23.1	23.0	23.0
6	2018-04-19	11:22:00	23.0	23.1	23.1
7	2018-04-19	11:24:00	23.1	23.1	23.1
8	2018-04-19	11:26:00	23.1	23.1	23.1
9	2018-04-19	11:28:00	23.2	23.2	23.2
10	2018-04-19	11:30:00	23.1	23.2	23.2
11	2018-04-19	11:32:00	23.2	23.3	23.3
12	2018-04-19	11:34:00	23.2	23.3	23.3
13	2018-04-19	11:36:00	23.2	23.4	23.4
14	2018-04-19	11:38:00	23.2	23.4	23.4
15	2018-04-19	11:40:00	23.2	23.4	23.4
16	2018-04-19	11:42:00	23.3	23.4	23.4
17	2018-04-19	11:44:00	23.3	23.4	23.4
18	2018-04-19	11:46:00	23.2	23.4	23.2
19	2018-04-19	11:48:00	23.3	23.4	23.2
20	2018-04-19	11:50:00	23.3	23.4	23.2
21	2018-04-19	11:52:00	23.3	23.4	23.4
22	2018-04-19	11:54:00	23.3	23.4	23.4
23	2018-04-19	11:56:00	23.2	23.3	23.2
24	2018-04-19	11:58:00	23.2	23.4	23.2
25	2018-04-19	12:00:00	23.3	23.3	23.3
26	2018-04-19	12:02:00	23.3	23.3	23.3
27	2018-04-19	12:04:00	23.2	23.2	23.2
28	2018-04-19	12:06:00	23.2	23.3	23.2
29	2018-04-19	12:08:00	23.2	23.2	23.2
30	2018-04-19	12:10:00	23.2	23.2	23.2
31	2018-04-19	12:12:00	23.2	23.2	23.2
32	2018-04-19	12:14:00	23.2	23.2	23.2
33	2018-04-19	12:16:00	23.2	23.2	23.2
34	2018-04-19	12:18:00	23.2	23.1	23.1
35	2018-04-19	12:20:00	23.2	23.2	23.2
36	2018-04-19	12:22:00	23.2	23.2	23.2
37	2018-04-19	12:24:00	23.2	23.1	23.1
38	2018-04-19	12:26:00	23.1	23.2	23.2
39	2018-04-19	12:28:00	23.1	23.2	23.2
40	2018-04-19	12:30:00	23.1	23.1	23.1
41	2018-04-19	12:32:00	23.1	23.1	23.1
42	2018-04-19	12:34:00	23.1	23.1	23.1

Data reports and data curves

Data reports and statistics

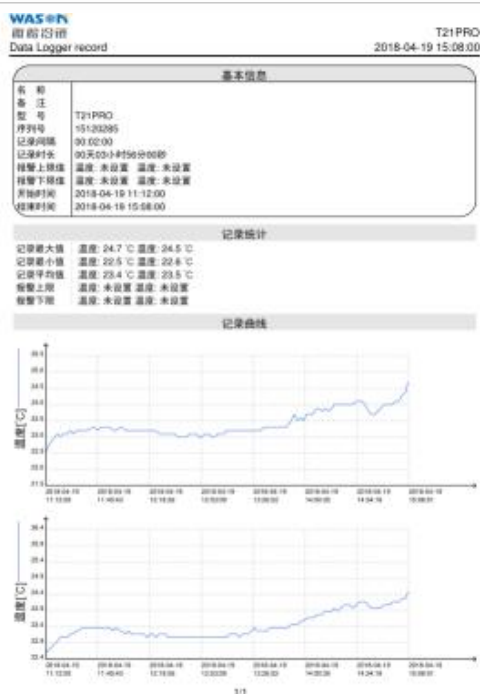

WASON 微松冷链
Data Logger record
T21PRO
2018-04-19 15:08:00

记录数据

序号	日期	时间	温度T1	温度T2	湿度
1	2018-04-19	11:00:00	22.5	22.2	22.8
2	2018-04-19	11:14:00	22.7	22.7	22.7
3	2018-04-19	11:16:00	22.8	22.8	22.8
4	2018-04-19	11:18:00	22.8	22.8	22.8
5	2018-04-19	11:20:00	23.1	23.0	23.0
6	2018-04-19	11:22:00	23.0	23.1	23.1
7	2018-04-19	11:24:00	23.1	23.1	23.1
8	2018-04-19	11:26:00	23.1	23.1	23.1
9	2018-04-19	11:28:00	23.2	23.2	23.2
10	2018-04-19	11:30:00	23.1	23.2	23.2
11	2018-04-19	11:32:00	23.2	23.3	23.3
12	2018-04-19	11:34:00	23.2	23.3	23.3
13	2018-04-19	11:36:00	23.2	23.4	23.4
14	2018-04-19	11:38:00	23.2	23.4	23.4
15	2018-04-19	11:40:00	23.2	23.4	23.4
16	2018-04-19	11:42:00	23.3	23.4	23.4
17	2018-04-19	11:44:00	23.3	23.4	23.4
18	2018-04-19	11:46:00	23.2	23.4	23.2
19	2018-04-19	11:48:00	23.3	23.4	23.2
20	2018-04-19	11:50:00	23.3	23.4	23.2
21	2018-04-19	11:52:00	23.3	23.4	23.4
22	2018-04-19	11:54:00	23.3	23.4	23.4
23	2018-04-19	11:56:00	23.2	23.3	23.2
24	2018-04-19	11:58:00	23.2	23.4	23.2
25	2018-04-19	12:00:00	23.3	23.3	23.3
26	2018-04-19	12:02:00	23.3	23.3	23.3
27	2018-04-19	12:04:00	23.2	23.2	23.2
28	2018-04-19	12:06:00	23.2	23.3	23.2
29	2018-04-19	12:08:00	23.2	23.2	23.2
30	2018-04-19	12:10:00	23.2	23.2	23.2
31	2018-04-19	12:12:00	23.2	23.2	23.2
32	2018-04-19	12:14:00	23.2	23.2	23.2
33	2018-04-19	12:16:00	23.2	23.2	23.2
34	2018-04-19	12:18:00	23.2	23.1	23.1
35	2018-04-19	12:20:00	23.2	23.2	23.2
36	2018-04-19	12:22:00	23.2	23.2	23.2
37	2018-04-19	12:24:00	23.2	23.1	23.1
38	2018-04-19	12:26:00	23.1	23.2	23.2
39	2018-04-19	12:28:00	23.1	23.2	23.2
40	2018-04-19	12:30:00	23.1	23.1	23.1
41	2018-04-19	12:32:00	23.1	23.1	23.1
42	2018-04-19	12:34:00	23.1	23.1	23.1

Output PDF curve

Output PDF report

Product Application:

It's widely used in different industries, such as food, pharmacy, electronics, chemicals, transportation, agricultural research, textiles, meteorological & environmental protection, HVAC refrigeration, archives management, and biochemical laboratory, etc.